VAGLIENTI BEAUTÉ

OVALIFT

Technology-enhanced massage device for face, neck and body



OVALIFT brings gua sha massage into a technology-enhanced treatment for the face and body. Microcurrents, EMS, warmth at 42 °C, intelligent vibration and LED light therapy are distributed across 3 targeted modes. Its curved surface follows larger areas, while its refined tip works precisely around contours.

Important

- Read this manual in full before first use and keep it for future reference.
- OVALIFT is a cosmetic device for personal use at home. It does not replace a medical device or advice from a healthcare professional.

- Use the device only on healthy, intact and non-irritated skin.
- Start at level 1, then increase gradually according to the comfort of your skin and the area treated.
- Never use the device while charging.
- OVALIFT is not waterproof. Do not rinse or immerse it or use it in a very humid environment.
- Do not look directly at the light source. Close your eyes when passing near the eye contour.
- Stop immediately if you experience pain, burning, persistent redness, dizziness or unusual discomfort.

1. Quick start

01
Charge the device
Fully charge OVALIFT before first use with the supplied USB-C cable.

02
Prepare the skin
Cleanse the area, then apply a conductive gel or skincare product that allows a smooth glide.

03
Switch on
Hold the on/off and mode button for about 2 seconds. OVALIFT starts in WARM at level 1.

04
Choose the mode
Briefly press on/off and mode to cycle from WARM to MSG, then MOIST.

05
Set the intensity
Start at level 1, then move to levels 2 or 3 if the sensation remains comfortable.

06
Place both contacts
In WARM and MOIST, keep the curved surface and tip against the skin at the same time.

07
Glide along the skin
Face: from the centre outwards and upwards. Body: longer movements.

08
Clean and store
Each mode lasts 10 minutes. Switch off, wipe the contacts and store in a dry place.

2. Device structure and contents

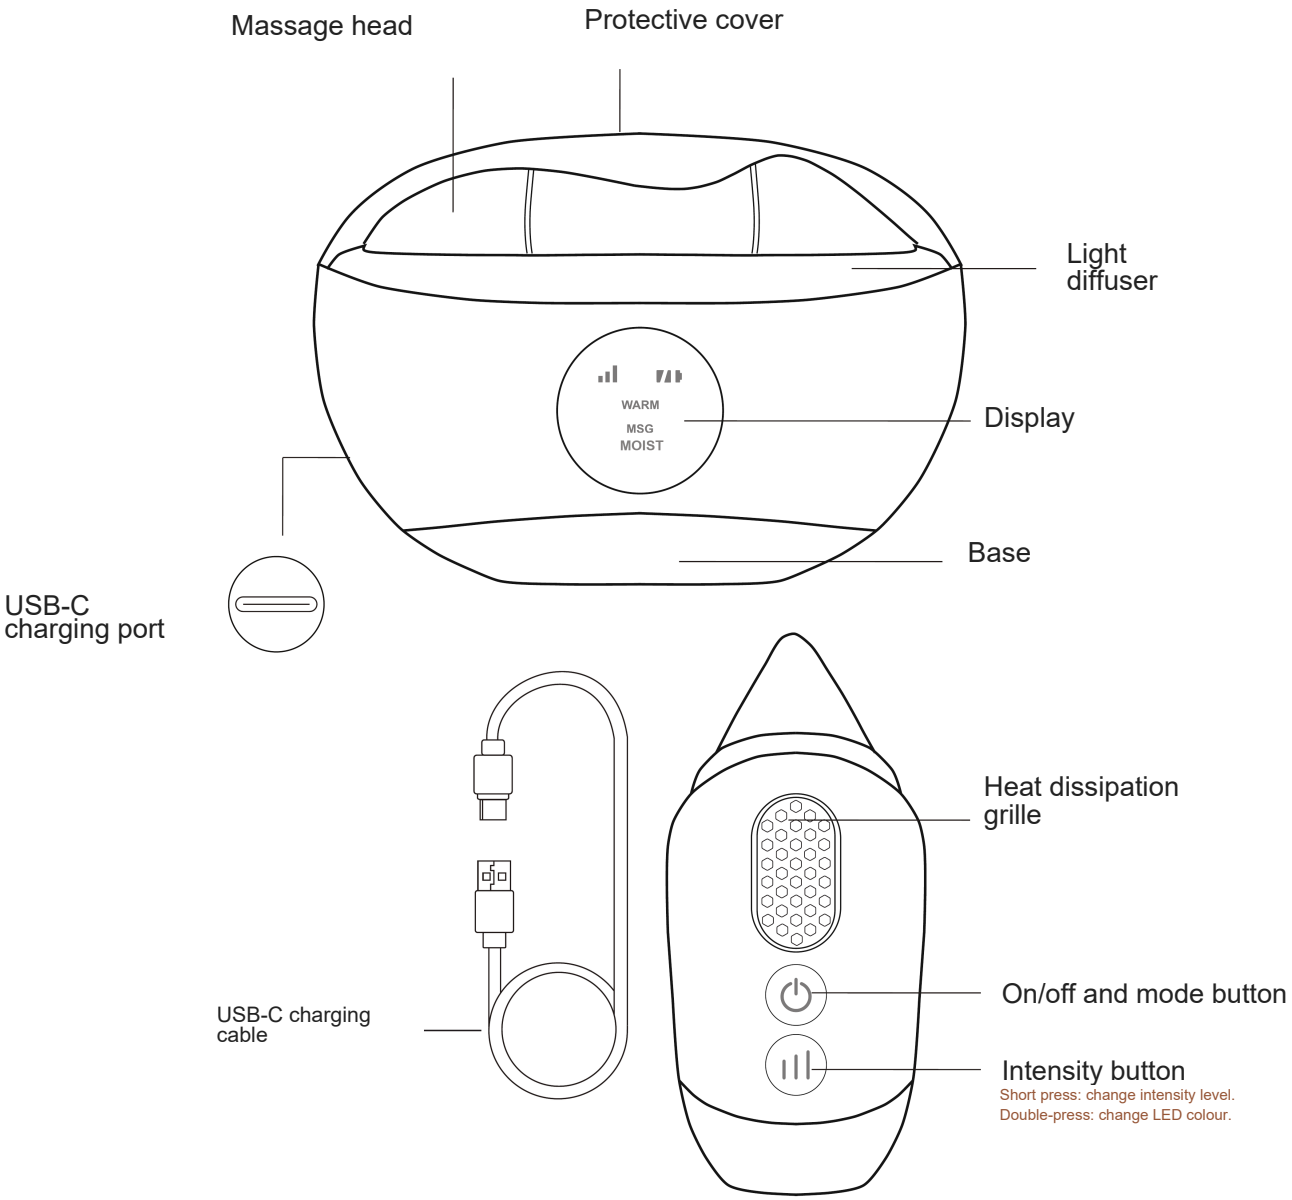

Box contents

OVALIFT device

A complete device for the face, neck and body.

USB-C cable

The USB-C charging cable is supplied with the device.

3. Main functions

Function	Setting	Role in the routine
Microcurrents	WARM, 3 levels	Gentle stimulation during the warming massage.
EMS	MSG and MOIST, 3 levels	A more pronounced pulse to support the appearance of toned tissue.
Warmth	42 °C, WARM and MOIST	Constant warmth during each pass.
Vibration	9,000 rpm, WARM and MOIST	Triggered when both conductive areas touch the skin at the same time.
LED light therapy	Red, blue and 7 colours in MOIST	Matches the light to the mode and treatment aim.

4. Controls, display and modes

Control	Action
On/off and mode	Hold for about 2 seconds to switch on or off. Press briefly to cycle through WARM, MSG and MOIST.
Intensity	Press briefly to cycle through levels 1, 2 and 3. The levels adjust the strength of the electrical pulse, never the temperature.
LED colours	In MOIST, double-press the intensity button to cycle through the LED colours.
Vibration	In WARM and MOIST, vibration starts automatically when both contacts touch the skin at the same time.

Reading the display

The bars on the left show the selected intensity level. The three segments on the right show the remaining battery level: they go out progressively as the battery runs down. The name shown in black is the active mode.



WARM

42 °C, microcurrents, contact-activated vibration and red LED 630 nm.



MSG

EMS, blue LED 470 nm; no warmth or vibration.



MOIST

42 °C, EMS, contact-activated vibration and 7 LED colours.

5. Step-by-step use

01

Create a smooth glide

Cleanse the area, then apply a product suited to conductivity and the chosen mode. For MOIST, use a serum, essence or formula that allows a continuous glide.

02

Choose the sensation

Choose WARM for warmth and microcurrents, MSG for a stronger EMS sensation or MOIST to work on the skin and applied formula at the same time.

03

Increase in stages

Start at level 1. Move to level 2, then level 3 when the area and your comfort allow.

04

Place both contacts

In WARM and MOIST, keep the curved surface and tip against the skin at the same time to trigger vibration.

05

Glide along the skin

Face: from the centre outwards and upwards. Body: longer movements that follow the curves.

06

Use for 10 minutes

Keep the device moving and return gradually to contours that need more precision.

Pressure and comfort

- Keep each movement slow, continuous and comfortable.
- Do not press hard or hold the metal head still on one area.
- Mild tingling or an occasional contraction may occur. Reduce the intensity if the sensation becomes unpleasant.
- Add more product if the glide lessens during a session.

6. Areas and movements

Area	Recommended movement
Face	Work from the centre outwards and upwards. Use the tip around contours and the curved surface on the cheeks and facial oval.
Neck	Make regular, gentle movements along the sides and back of the neck. Avoid excessive pressure.
Arms and hands	Follow the muscle lines with slow, continuous passes.
Waist and hips	Use the curved surface for broad movements that follow the body's curves.
Legs	Glide upwards in long strokes without lingering on sensitive or painful areas.
Back	Ask another person to guide the device if you cannot reach the area without strain or twisting.

7. The 7 LED colours in MOIST mode

Colour	Wavelength	Aim
Red	630 nm	Age-defying, smooths wrinkles.
Yellow	590 nm	Radiance, revives the complexion.
Green	550 nm	Harmony, evens the complexion.
Cyan	490 nm	Comfort, soothes sensitivity.
Blue	470 nm	Clear-looking skin, purifies the skin.
Violet	420 nm	Targeted purity, targets blemishes.
White	-	All-round care, revives the overall appearance.

8. Recommended frequency

01

First use

Start at level 1 to observe the skin's reaction and the electrical sensation.

02

Progression

Move to levels 2 then 3 only when the previous level remains comfortable.

03

Duration

Each mode offers a 10-minute cycle.

04

Frequency

Healthy skin that tolerates the device well can progress to a daily session. Start gradually.

05

After the session

Switch off the device, remove excess product if necessary and continue with your usual skincare.

9. Charging



- Switch off OVALIFT. Never use the device while charging.
- Check that the USB-C port and cable are completely dry.
- Connect the supplied USB-C cable to the device, then to a suitable USB power supply.
- The indicator flashes while charging and remains lit when the battery is full.
- A full charge takes approximately 2 hours.
- Disconnect the cable when charging is complete.

10. Cleaning, care and storage

- Switch off and unplug the device before cleaning.
- Wipe the metal head and external surfaces with a slightly damp soft cloth.
- Carefully remove all gel, serum, essence or skincare residue after each use.
- Thoroughly dry the device and USB-C port before storage or charging.
- Do not rinse or immerse OVALIFT or clean it under running water.
- Do not use harsh alcohol, solvents, abrasive products or corrosive detergents.
- Do not drop, strike, pierce, disassemble or modify the device.
- Store OVALIFT in a dry, clean place at a moderate temperature, out of reach of children.

11. Precautions and contraindications

- Do not use on a wound, open lesion, burn, infection, active inflammation or painful area.
- Do not use with a pacemaker, implanted medical device or electronic implant without medical advice.
- If you are pregnant or have epilepsy, heart disease, cancer, a significant blood pressure disorder, ongoing medical treatment or any doubt, seek advice from a healthcare professional before use.
- Do not use if you have a fever, acute illness or feel too unwell for a comfortable treatment.
- Do not look directly at the light. Close your eyes when the head approaches the eye contour.
- Remove jewellery and metal accessories near the area being treated.
- Do not use with a damaged cable, after a serious fall, or if there is a crack, unusual smell or overheating.

- Switch off the device immediately if it becomes unusually hot to avoid burns.
- Children must not use the device. Keep OVALIFT and its cable out of their reach.

12. Quick troubleshooting

Situation	Possible causes	What to do
The device does not turn on	Flat battery or button held too briefly.	Charge OVALIFT, then hold on/off and mode for about 2 seconds.
The intensity feels weak or uneven	Incomplete contact, insufficient product or level too low.	Reposition both contacts, add product and gradually adjust the intensity.
Vibration stops during movement	One of the two conductive areas is no longer touching the skin.	Adjust the angle so that the curved surface and tip stay in contact together.
Vibration does not work in MSG	Normal operation.	Vibration works only in WARM and MOIST.
Warmth is not felt in MSG	Normal operation.	MSG works at ambient temperature, without warmth.
The electrical sensation is too strong	High intensity, sensitive skin or insufficient glide.	Return to level 1, add product and stop if discomfort persists.
The device does not charge	Loose cable, unsuitable power supply or damp port.	Check connections, dry the USB-C port and try again.

13. Technical specifications

Item	Data
Product name	OVALIFT
Areas	Face, neck and body
EMS frequency	2,900 Hz
Modes	WARM, MSG, MOIST
Intensity levels	3 levels for each mode
LED	Red 630 nm, yellow 590 nm, green 550 nm, cyan 490 nm, blue 470 nm, violet 420 nm, white
Warmth	42 °C, WARM and MOIST modes
Vibration	9,000 rpm, activated by contact with the skin
Session	10 minutes per mode
Battery	600 mAh
Charging	USB-C, approximately 2 hours
Protection	Not waterproof; do not rinse or immerse
Dimensions	116 x 80 x 36 mm
Weight	128 g
Box contents	OVALIFT device, USB-C charging cable

14. Recycling, guarantee and service

At the end of its life, do not dispose of OVALIFT with household waste. Take it to a suitable collection point for electrical and electronic equipment.

OVALIFT comes with a two-year commercial guarantee from the date of purchase, provided it is used in accordance with this manual.

The guarantee does not cover damage caused by dropping, immersion, disassembly, modification, an unsuitable power supply or non-compliant use.

15. Entity responsible for EU market placement

Item	Information
Entity placing on EU market	Vaglienti Beauté
Postal address	1055 Budapest, Szent István körút 27., 1. em. 7. ajtó, Hungary
Contact	support@vaglienti-beaute.com
Product page	https://vaglienti-beaute.com/ovalift.html

Scan the QR code for the OVALIFT product page, usage advice and updated information.